

CONFIGURATION OF TEST CHIP

- Primers and probe for N gene of SARS-CoV-2
- Primers and probe for RdRP gene of SARS-CoV-2
- For running No template control
- For running Positive control

*Each well includes a internal positive control

WORKFLOW

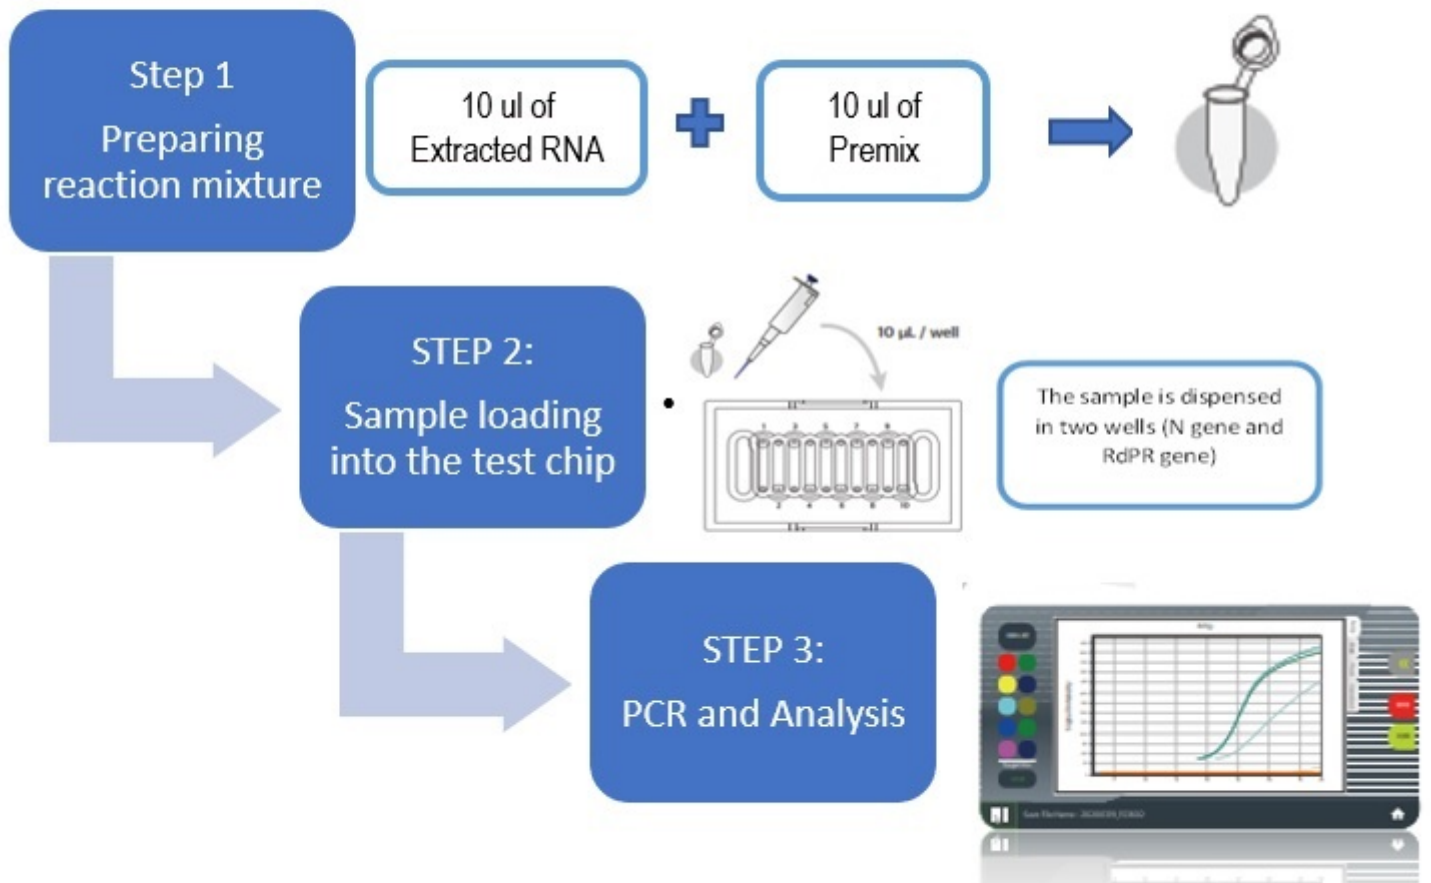


Fig. S1. Workflow of RT-qPCR SMARTCHECK