


Additional file 2: IC₅₀ calculations for positive human pAb

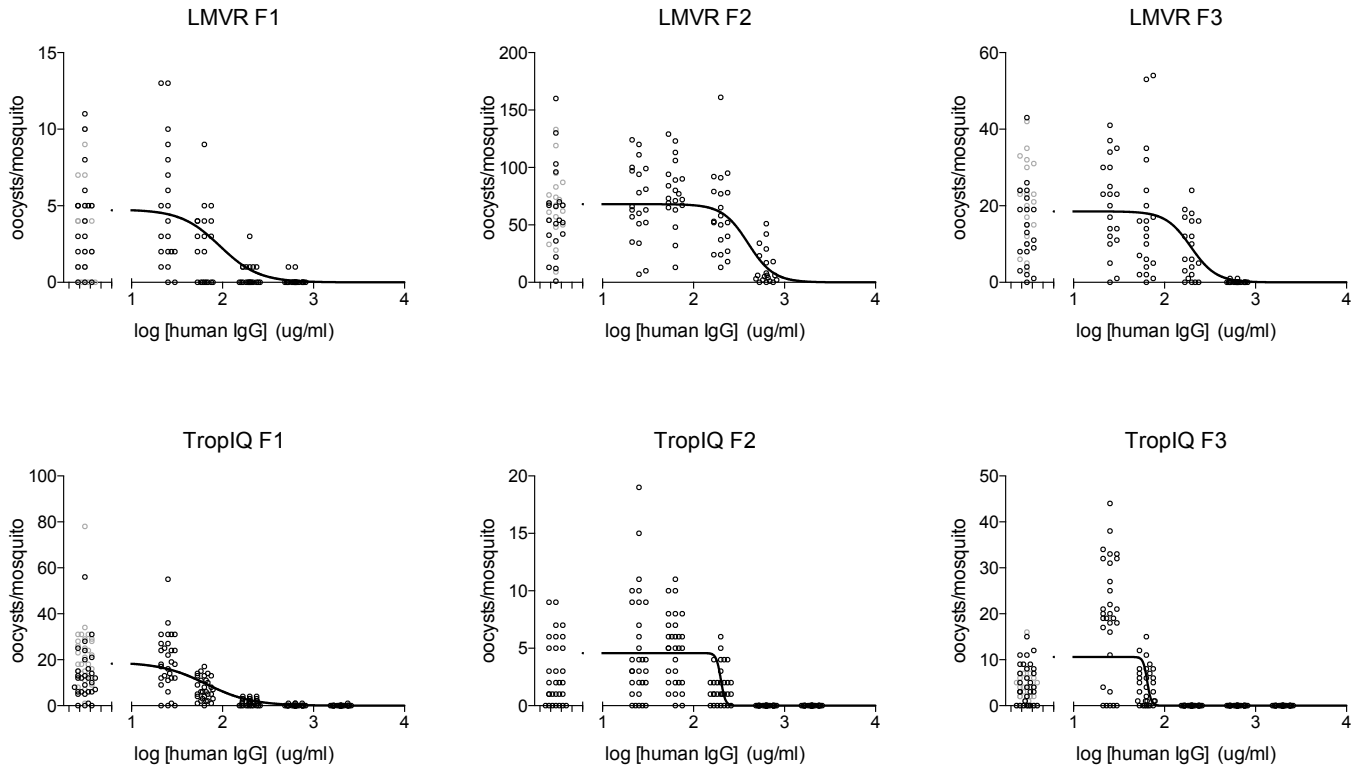

In both laboratories, positive human IgG was tested at 23, 70, 10.4, 210 and 630 $\mu\text{g/ml}$ in three feeding experiments (F1, F2 and F3). Oocyst count in each mosquito and the best fit to a Hill equation are shown.