




### Normal Cycle

### Cycle with automated P0.1 measurement

A Löwenstein Medical Elisa 800®

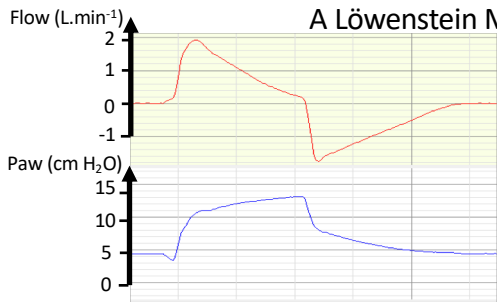

B Getinge Group Servo-u®

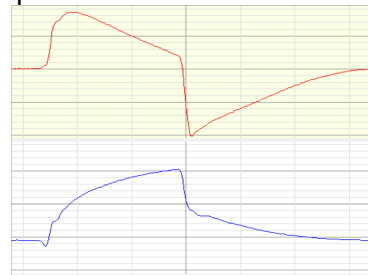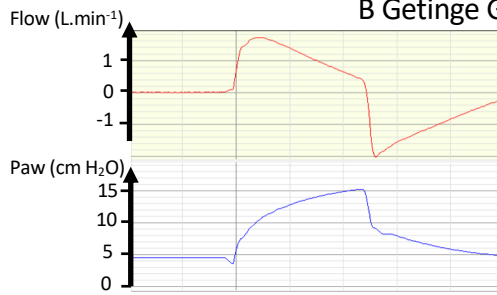

0.4 s

