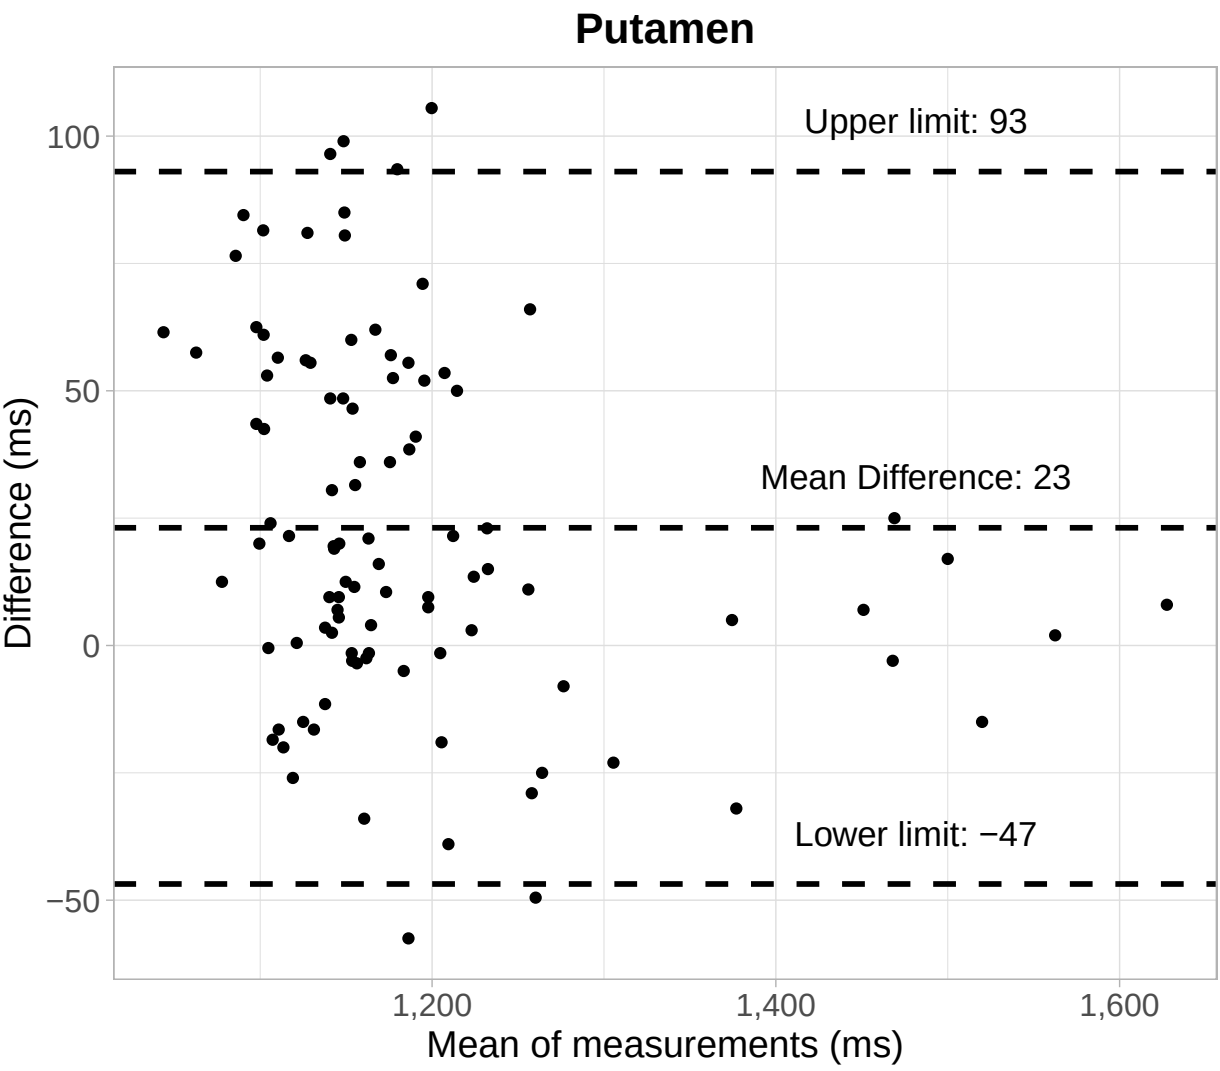
Putamen
Upper limit: 93
Mean Difference: 23
Lower limit: −47
100
50
0
−50
Difference (ms)
1,200
1,400
1,600
Mean of measurements (ms)