


10 saliva samples



Pipetting 20 μ L of each sample to the same eppendorf

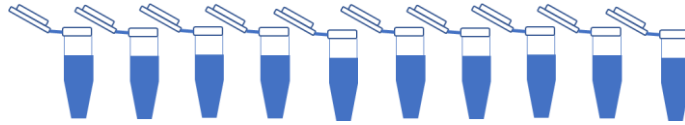

Saliva pool (200 μ L)



Pool DNA Extraction + Real Time PCR Reaction



POSITIVE RESULT

Pipetting 200 μ L of each sample to an eppendorf



DNA Extraction + Real Time PCR Reaction of the 10 samples



Positive(s) sample(s) for HCMV DNA are identified

NEGATIVE RESULT



All 10 saliva samples are negative
for HCMV DNA